



## CALYS 1500

Advanced laboratory electrical calibrator / Dual input thermometer

Representative



特旺通科藝私營有限公司  
THERMOTRON-CE TECHNOLOGY PTE LTD

10 Bukit Batok Crescent #05-03 The Spire, Singapore 658079 | T (65)6896 1586 | WA (65)9829 4363  
www.thermotron-ce.com.sg | sales@thermotron-ce.com.sg | mailbox@thermotron-ce.com.sg

CALYS 1500, most advanced and accurate laboratory electrical calibrator of the range, does not only work as a simulator (IN / OUT) but also as a dual channel thermometer (IN / IN) to perform comparison calibration. It calibrates HART transmitters (HART communicator) and thermistors.

## Description

CALYS 1500, most advanced and accurate laboratory electrical calibrator of the range, does not only work as a simulator (IN / OUT) but also as a dual channel thermometer (IN / IN) to perform comparison calibration. It calibrates HART transmitters (HART communicator) and thermistors. It is the perfect tool for advanced process maintenance and use on test bench in all industries. Suitable for all field and lab measurements, it can simultaneously measure and generate over two isolated channels various signals of temperature, resistance, process, pressure and frequency in one single instrument. Providing **extended functionalities** (temperature simulation, scaling, steps, synthesizer, statistical functions...) and audit trails, CALYS 1500 complies with both 21 CFR Part 11 and NADCAP Heat Treatment standards and makes advanced data exploitation and full data traceability easier. 10 full configurations can be saved and recalled by the user or the user group, making CALYS 1500 the ideal tool for regular and repeated tasks. High performances in measurement and simulation for CALYS 1500:

- Temperature Up to 0.005 % RDG
- Resistance Up to 0.006 % RDG and 50 K $\Omega$  range
- Current: Up to 0.007 % RDG and 100 mA range + Loop Supply 24 V
- Voltage: Up to 0.005 % RDG and 50 V range
- Frequency: Up to 0.01 % RDG and 100 KHz range
- Pressure: With an external pressure module (comparison calibration with a pressure pump)

## Calibration procedures and DATACAL software

Using this user-friendly instrument, calibration tasks can be quickly carried out over the whole process chain. Take the documenting process calibrator to the field with you during the whole week with 10 calibration procedures stored in the device. Run the procedure after connecting the probes to the instrument and save the results for onsite easy and quick calibration. Back to the office, you can then upload the data on a computer in order to issue customized calibration certificates with dedicated calibration software DATACAL.


### Innovative and ergonomic design

- Metal housing for enhanced robustness
- Capacitive touch panel
- USB communication
- Carrying handle

- Battery and main powered

## Graphic screen and display resolution

CALYS 1500 allows the digit number after the dot to be selected: This function is justified by the needs of users who want or not to display the best resolution for calibration or on the contrary limit it for simple verifications. CALYS 1500 dual display indicates permanently the measurement value, and also the emitted value, the gauge and the used functions. On the top date, time and also external temperature are also indicated. During measuring average, maximum, minimum and the number of measurements are displayed on the left. While for emission this part of screen displays all details of ramps, steps and constant value emission functions. Drop-down menus are used with the navigator, and an on-line help is available to make easier connections of probes and wires.

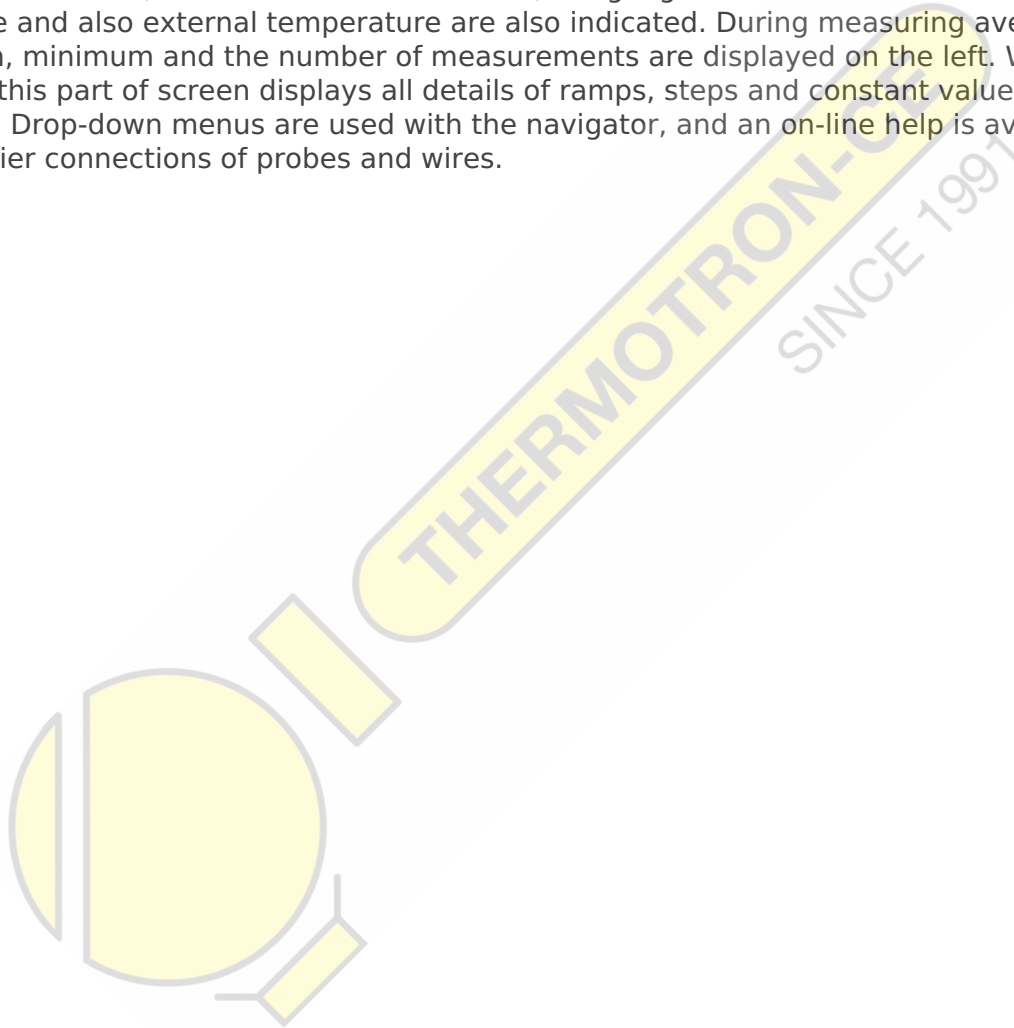

# Specifications

## Specifications and performances in temperature @23°C ±5°C

Uncertainty is given in % of reading (CALYS 1500 display) + fixed value.

### Resistive probes: Measurement and simulation

Sensor	Range (Input and Output)	Resolution	Accuracy / 1 year (Measurement)	Accuracy / 1 year (Simulation)
Pt50 ( $\alpha = 3851$ )	-220°C to +850°C	0.01°C	0.006% RDG + 0.04°C	0.006% RDG + 0.04°C
Pt100 ( $\alpha = 3851$ )	-220°C to +850°C	0.01°C	0.006% RDG + 0.03°C	0.006% RDG + 0.035°C
Pt100 ( $\alpha = 3916$ )	-200°C to +510°C	0.01°C	0.006% RDG + 0.03°C	0.006% RDG + 0.035°C
Pt100 ( $\alpha = 3926$ )	-210°C to +850°C	0.01°C	0.006% RDG + 0.03°C	0.006% RDG + 0.035°C
Pt200 ( $\alpha = 3851$ )	-220°C to +850°C	0.01°C	0.006% RDG + 0.04°C	0.006% RDG + 0.04°C
Pt500 ( $\alpha = 3851$ )	-220°C to +850°C	0.01°C	0.006% RDG + 0.03°C	0.006% RDG + 0.04°C
Pt1000 ( $\alpha = 3851$ )	-220°C to +740°C	0.01°C	0.006% RDG + 0.03°C	0.006% RDG + 0.035°C
Ni100 ( $\alpha = 618$ )	-60°C to +180°C	0.01°C	0.006% RDG + 0.05°C	0.006% RDG + 0.04°C
Ni120 ( $\alpha = 672$ )	-40°C to +205°C	0.01°C	0.006% RDG + 0.05°C	0.006% RDG + 0.04°C
Ni1000 ( $\alpha = 618$ )	-60°C to +180°C	0.01°C	0.006% RDG + 0.05°C	0.006% RDG + 0.04°C
Cu10 ( $\alpha = 427$ )	-50°C to +150°C (Mes) -70°C to +150°C (Sim)	0,10°C (Mes) 0.01°C (Sim)	0.006% RDG + 0.18°C	0.006% RDG + 0.1°C
Cu50 ( $\alpha = 428$ )	-50°C to +200°C	0.01°C	0.006% RDG + 0.05°C	0.006% RDG + 0.05°C

Temperature coefficient: < 10% of accuracy /°C beyond reference domain Resistive probes measurements in 2, 3 or 4 wires: automatic recognition of number of connected wires, with indication on screen Accuracies are given for 4-wire mounted probes Take into account particular error of temperature sensor used and implementation conditions Admissible measuring current: 0.25 mA (Measurement) or 0.1 mA to 1 mA (Emission)

### Thermocouples: Measurement and simulation

Type	Input range	Resolution	Accuracy / 1 year (Measurement)	Output range	Resolution	Accuracy / 1 year (Simulation)
K	-250 to -200°C -200 to -120°C -120 to +1372°C	0.10°C 0.05°C 0.01°C	0.50°C 0.15°C 0.005% RDG + 0.08°C	-250 to -50°C -50 to +120°C +120 to +1020°C +1020 to +1370°C	0.01°C 0.01°C 0.01°C 0.01°C	0.15% RDG 0.06°C 0.005% RDG + 0.05°C 0.007% RDG + 0.05°C
T	-250 to -200°C -200 to -100°C -100 to +80°C +80 to +400°C	0.1°C 0.01°C 0.01°C 0.01°C	0.50°C 0.05% RDG + 0.06°C 0.015% RDG + 0.07°C 0.06°C	-250 to -100°C -100 to +0°C +0 to +400°C	0.01°C 0.01°C 0.01°C	0.1% RDG + 0.05°C 0.02% RDG + 0.06°C 0.055°C
J	-210 to -120°C -120 to +60°C +60 to +1200°C	0.01°C 0.01°C 0.01°C	0.15°C 0.005% RDG + 0.07°C 0.0025% RDG + 0.06°C	-210 to -0°C +0 to +50°C +50 to +1200°C	0.01°C 0.01°C 0.01°C	0.03% RDG + 0.08°C 0.05% RDG + 0.07°C 0.005% RDG + 0.04°C
E	-250 to -200°C -200 to +100°C +100 to 1000°C	0.05°C 0.01°C 0.01°C	0.30°C 0.06°C 0.005% RDG + 0.05°C	-250 to +40°C +40 to +550°C +550 to +1000°C	0.01°C 0.01°C 0.01°C	0.15°C 0.005% RDG + 0.12°C 0.005% RDG + 0.13°C
R	-50 to +150°C +150 to +550°C +550 to 1768°C	0.2°C 0.1°C 0.01°C	0.60°C 0.30°C 0.30°C	-50 to +0°C +0 to +350°C +350 to 1768°C	0.01°C 0.01°C 0.01°C	0.35% RDG + 0.4°C 0.04°C 0.25°C
S	-50 to +150°C +150 to +550°C +550 to +1450°C +1450 to +1768°C	0.20°C 0.10°C 0.05°C 0.05°C	0.80°C 0.30°C 0.30°C 0.35°C	-50 to +0°C +0 to +350°C +350 to +1768°C	0.01°C 0.01°C 0.01°C	0.25% RDG + 0.4°C 0.30°C 0.25°C
B	+400 to +900°C +900 to +1820°C	0.1°C 0.05°C	0.005% RDG + 0.4°C 0.005% RDG + 0.2°C	+400 to +900°C +900 to +1820°C	0.01°C 0.01°C	0.005% RDG + 0.4°C 0.005% RDG + 0.2°C
U	-200 to -100°C -100 to +660°C	0.01°C 0.01°C	0.13°C 0.09°C	-200 to +400°C +400 to +660°C	0.05°C 0.05°C	0.09°C 0.11°C

L	-200 to +900°C	0.01°C	0.10°C	-200 to +900°C	0.05°C	0.15°C
C	-20 to +900°C +900 to +1730°C +1730 to °C	0.05°C 0,05°C 0,05°C	0.15°C 0.008% RDG + 0.12°C 0.015% RDG + 0.12°C	-20 to +1540°C +1540 to +2310°C	0.10°C 0.10°C	0.25°C 0.012% RDG + 0.1°C
N	-240 to -190°C -190 to -110°C -110 to +0°C +0 to 400°C +400°C to +1300°C	0,10°C 0.05°C 0.01°C 0.01°C 0.01°C	0.25% RDG 0.10% RDG 0.04% RDG + 0.06°C 0.08°C 0.005% RDG + 0.06°C	-240 to -200°C -200 to +100°C +10 to +250°C +250 to +1300°C	0.01°C 0.01°C 0.01°C 0.01°C	0.15% RDG 0.10°C 0.08°C 0.008% RDG + 0.05°C
Platine	-100 to +100°C +100 to +1400°C	0.01°C 0.01°C	0.15°C 0.005% RDG + 0.06°C	-100 to +1400°C	0.05°C	0.10°C
Mo	+0 to +1375°C	0.01°C	0.005% RDG + 0.06°C	+0 to +1375°C	0.05°C	0.005% RDG + 0.06°C
NiMo/NiCo	-50 to +1410°C	0.01°C	0.005% RDG + 0.30°C	-50 to +1410°C	0.05°C	0.005% RDG + 0.3°C

Temperature coefficient: < 5% of accuracy /°C beyond reference domain Accuracy is given for reference @ 0°C. When using the internal reference junction (except couple B) add an additional uncertainty of 0.2 °C at 0 °C. It is possible (thermocouple B excepted) to choose by programming the cold junction localization: External at 0°C, internal (temperature compensation of instrument's terminals) or manually entered. Display unit: °C? F and K. Thermocouples: G, D: For specifications, refer to the instruction manual (Available on request)

### Specifications and performances in pressure @23°C ±5°C



#### **Pressure: Measurement by external digital sensor**

Range	0-1 bar	0-3 bar	0-10 bar	0-30 bar	0-100 bar	0-300 bar	0-1000 bar
Absolute	X	X	X	X	X	X	X
Relative	X	X	X	X			

Available in relative, absolute and differential pressure. Connector: ¼ gas Resolution: 0.02% FS Accuracy: -0.05% FS from 10 to 40°C - 0.1% FS from -10 to +10°C and from 40 to 80°C This

digital pressure module ACL433 is connected to CALYS 1500 through RS485 serial cable to the digital input connector. All data are digital. Measurements are compensated in temperature by a polynomial correction implemented into the firmware at factory.

## Specifications and performances in process @23°C ±5°C

### DC current: Measurement

With or without loop supply

Range	Resolution	Accuracy / 1 year	Nota: Rin
0-20 mA	0.1 µA	0.007% RDG + 0.8 µA	< 30 Ω
4-20 mA	0.1 µA	0.007% RDG + 0.8 µA	< 30 Ω
±100 mA	0.1 µA	0.007% RDG + 2 µA	< 30 Ω

Temperature coefficient: < 7% of accuracy /°C beyond reference domain Loop supply: 24 V ±10% HART® compatibility: Input impedance Rin = 280 Ω CALYS 1500 also allows linear or quadratic signals to be linearized. Specifications given for CALYS configurations in: - Active mode (+24V ON) 1 Meter in passive mode (+24 V OFF) - Passive mode (+24 V OFF) 1 Meter in active mode (+24 V ON)

### Direct voltage: Measurement

Range	Full range	Resolution	Accuracy / 1 year	Nota: Rin
100 mV	-10 mV to 100 mV	1 µV	0.005% RDG + 2 µV	> 10 MΩ
1 V (1)	-100 mV to 1 V	10 µV	0.005% RDG + 8 µV	> 10 MΩ
10 V	-1 V to 10 V	100 µV	0.007% RDG + 80 µV	= 1 MΩ
50 V	-5 V to 50 V	1 mV	0.007% RDG + 0.5 mV	= 1 MΩ

Temperature coefficient: < 5% of accuracy /°C beyond reference domain

### Frequency and counting: Measurement

Range	Full range	Resolution	Accuracy / 1 year
10 KHz	1 Hz to 10 KHz	0.1 Hz	0.005% RDG + 5 mHz
100 KHz	10 Hz to 100 KHz	0.1 Hz	0.005% RDG + 5 mHz

Temperature coefficient: < 5 ppm/°C beyond reference domain Scale unit: Pulse / min and Hz Trigger level: 1 V Measurement on frequency signals or dry contacts Counting will be performed on defined time or infinite time

### Resistance: Measurement

Range	Resolution	Accuracy / 1 year	Nota: Rin

Range	Resolution	Accuracy / 1 year
400 $\Omega$	1 m $\Omega$	0.006% RDG + 8 m $\Omega$
3600 $\Omega$	10 m $\Omega$	0.006% RDG + 50 m $\Omega$
50 K $\Omega$ (1)	100 m $\Omega$	0.008% RDG + 1 $\Omega$

(1) Range on channel 1 only. Temperature coefficient: < 7 ppm/ $^{\circ}$ C beyond reference domain 2, 3 or 4 wires resistance measurement: automatic recognition of number of connected wires, with indication on screen Accuracies are given for 4-wire mounted probes Open circuit terminal voltage: < 10 V Continuity test: Open circuit for R > 1000  $\Omega$  and closed circuit for R < 1000  $\Omega$

### DC current: Emission

Calibre	Résolution	Précision / 1 an	Note
24 mA	1 $\mu$ A	0,007% L + 0,8 $\mu$ A	With or without loop supply (24 V)
4-20 mA	1 $\mu$ A	0,007% L + 0,8 $\mu$ A	
0-20 mA	1 $\mu$ A	0,007% L + 0,8 $\mu$ A	

Temperature coefficient: < 7 ppm/ $^{\circ}$ C beyond reference domain Settling time: < 5 ms Specifications given for CALYS configurations in: - Active mode (+24V ON) 1 Meter in passive mode (+24 V OFF) - Passive mode (+24 V OFF) 1 Meter in active mode (+24 V ON) Pre-programmed steps

	0%	25%	50%	75%	100%
4-20 mA linear	4	8	12	16	20
0-20 mA linear	0	5	10	15	20
4-20 mA quad	4	5	8	13	20
0-20 mA quad	0	1.25	5	11.25	20
4-20 mA valves	3.8-4-4.2		12		19, 20, 21

### Direct voltage: Emission

Range	Full range	Resolution	Accuracy / 1 year	Minimum output load
100 mV	-5 mV to 100 mV	1 $\mu$ V	0.005% RDG + 2 $\mu$ V	1 K $\Omega$
1 V	-5 mV to 1 V	10 $\mu$ V	0.005% RDG + 8 $\mu$ V	2 K $\Omega$
10 V	-100 mV to 10 V	100 $\mu$ V	0.007% RDG + 80 $\mu$ V	4 K $\Omega$
50 V	-100 mV to 50 V	1 mV	0.007% RDG + 0.5 mV	4 K $\Omega$

Temperature coefficient: < 5 ppm/ $^{\circ}$ C beyond reference domain

### Frequency and pulses: Emission

Range	Resolution	Accuracy / 1 year
1000 Hz	0.01 Hz	0.005% RDG + 5 mHz
100 KHz	1 Hz	0.005% RDG + 5 mHz

Temperature coefficient: < 5 ppm/°C beyond reference domain Scale unit: Pulse / min and Hz  
Pulse emission and dry contact simulation Max amplitude: 20 V selectable by user

### Resistance: Emission

Range	Full range	Resolution	Accuracy / 1 year	Notes
400 Ω - 1 mA (Direct current)	1 Ω to 400 Ω	10 mΩ	0.006% RDG + 20 mΩ	lext : 0.1 mA - 1 mA
400 Ω - 1 mA (Pulsed current)	1 Ω to 400 Ω	10 mΩ	0.006% RDG + 30 mΩ	lext : 0.1 mA - 1 mA
400 Ω - 4 mA (Direct current)	1 Ω to 400 Ω	10 mΩ	0.006% RDG + 20 mΩ	lext : 1 mA - 4 mA
400 Ω - 4 mA (Pulsed current)	1 Ω to 400 Ω	10 mΩ	0.006% RDG + 30 mΩ	lext : 1 mA - 4 mA
3600 Ω (Direct current)	10 Ω to 3600 Ω	100 mΩ	0.006% RDG + 100 mΩ	lext : 0.1 / 1 mA
3600 Ω (Pulsed current)	10 Ω to 3600 Ω	100 mΩ	0.006% RDG + 200 mΩ	lext : 0.1 / 1 mA

Temperature coefficient: < 5 ppm/°C beyond reference domain lext : Current received by the calibrator

### Further functionalities

File Menu

Users can save up to 10 full configurations of the instruments and recall them. Configurations include all programming done on instrument.

Scaling in measurement and simulation modes

Scaling allows process signals to be displayed in % of FS or in all other units. This function also allows sensors to be corrected after a calibration.

Relative measurement

## Models and accessories

### Instrument:

CALYS 1500 Benchtop precision documenting multifunction calibrator Delivered in standard with:

- Quick start manual
- Battery charger
- Set of 6 testing leads
- Factory test report

### Accessories:

ACL433 External digital pressure sensor, range to be specified at the order: Absolute or relative pressure: Range from -1 -> 1; 3; 10; 30 bar Absolute pressure: Range from -1 -> 100; 300; 1000 bar  
ACL9311 Set of 6 measuring cables with removable crocodile clips  
ER 49504-000 USB cable  
ACL500 Hart modem for CALYS 150  
ACL600 Cable to drive temperature dry blocks and baths for CALYS 150 *Please ask before for compliance with your bath / dry-block*

### Logiciel :

### Software:

DATA CAL Calibration software for CALYS 1000 / 1200 / 1500 Supplied with USB cable

### Certification:

QMA11EN COFRAC certificate of calibration With all relevant data points where the device has been tested  
AMS 2750 Compliance certificate to NADCAP AMS 2750 standard

### Packing information:

Size 340 x 320 x 160 mm Weight without packing 4,6 Kg